


U s a U U f n f U s U s A U s n f
U U U s n
u h #
h #
u




Superior oxygen and moisture barrier properties
Proven design for Gamma and ETO sterilization processes
Controlled dispensing, no overflow, no suck back minimizing contaminants

GMP facility
Drug Master File (DMF)
ISO:9001 Certification

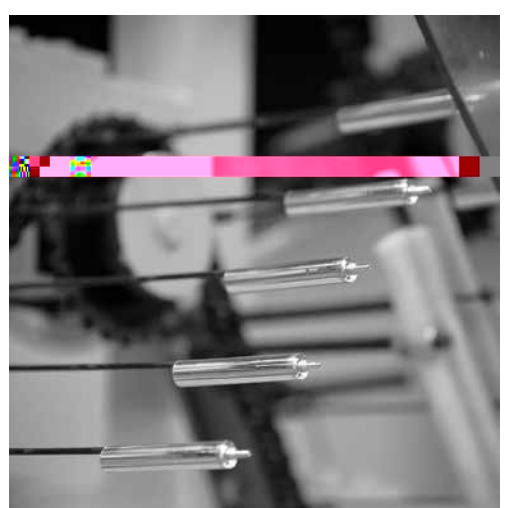

Fill capacity- 1g to 3.5g (available up to 5g)
Patented tamper evident closure system
In-house pre-press and Flexographic printing up to 4 colors

Size 1/2" (13mm) diameter available
Ophthalmic tip

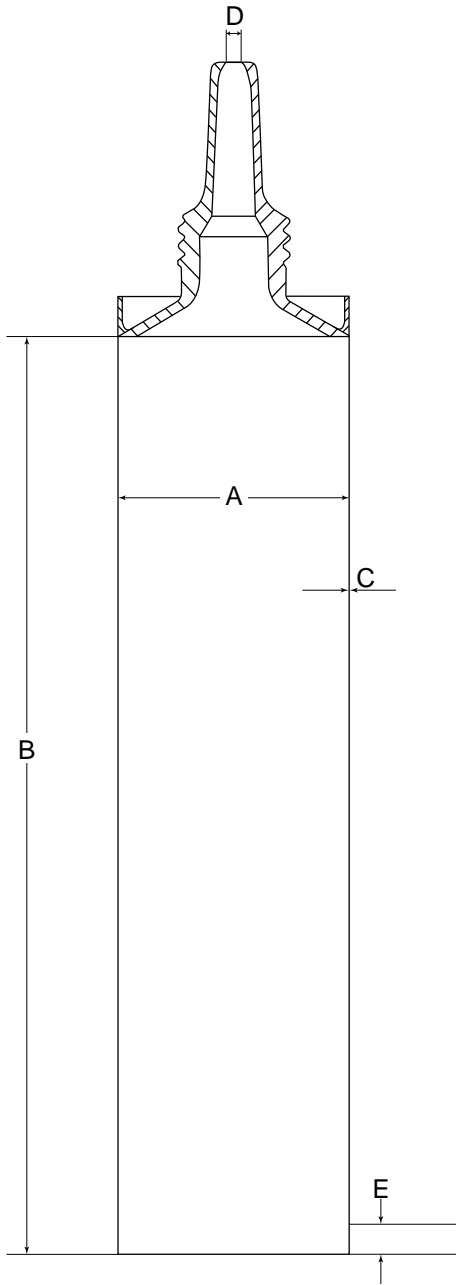

	DIMENSION	TARGET	MAXIMUM	MINIMUM
A	Tube Diameter	0.500	0.505	0.495
B	Length - Standard for 1G	2.000	2.031	1.969
	Standard for 3G fill	2.750	2.781	2.719
C	Wall Thickness	0.0044	0.0055	0.0033
D	Orifice	0.050	0.060	0.045
E	Bare Metal Margin *	0.656	0.687	0.625

*PCH requires a minimum of 0.0625 inches of bare metal. The standard for a 2.750 length tube is 0.656 inches. However, this can be modified to meet customer requirements.

NOT TO SCALE



4850 Crowe Drive
Mount Crawford, VA 22841

Fax (540) 434-6462

(540) 434-4411

DESCRIPTION:

Eye Tip Tin Tube 0.500in. Dia.
Tamper Evident

DRAWING No.:

GEN-002

CUSTOMER APPROVAL:

DATE:

This is a CONTROLLED DOCUMENT and is considered PROPRIETARY information of
Reproductions of this document are considered uncontrolled and will not be updated.

, Inc.

EPS 02/26/20